

Yocom-McColl Testing Laboratories, Inc.
 540 West Elk Place • Denver, Colorado 80216-1823 USA
 PHONE (303) 294-0582 • FAX (303) 295-6944
 EMAIL: ymccoll@ymccoll.com

**Optical Fiber Diameter Analyser (OFDA100)
 Micron Test Report**

Lodi Alpacas/Jan Clingman
 W12002 Slack Road
 Lodi WI 53555 USA

06/24/10


Test No: 379780

Animal and Sample Description

Animal Name: SSR Dura Lock	Animal ID: 1098594
Breed: Alpaca(Suri)	Sample Location: Side
Sex: Male	Sample Date: 05/09/10
Color: White	Age: 10/28/05

Laboratory Data

Mean Fiber Diameter: 28.1 microns	Spin Fineness: 26.8 microns
Standard Deviation: 5.2 microns	Mean Curvature (deg/mm): 8.9
Coefficient of Variation: 18.7 %	SD Curvature (deg/mm): 15.1
Fibers Greater Than 30 microns: 29.5 %	Comfort Factor: 70.5 %
Medullated Fibers: 22.9 %	

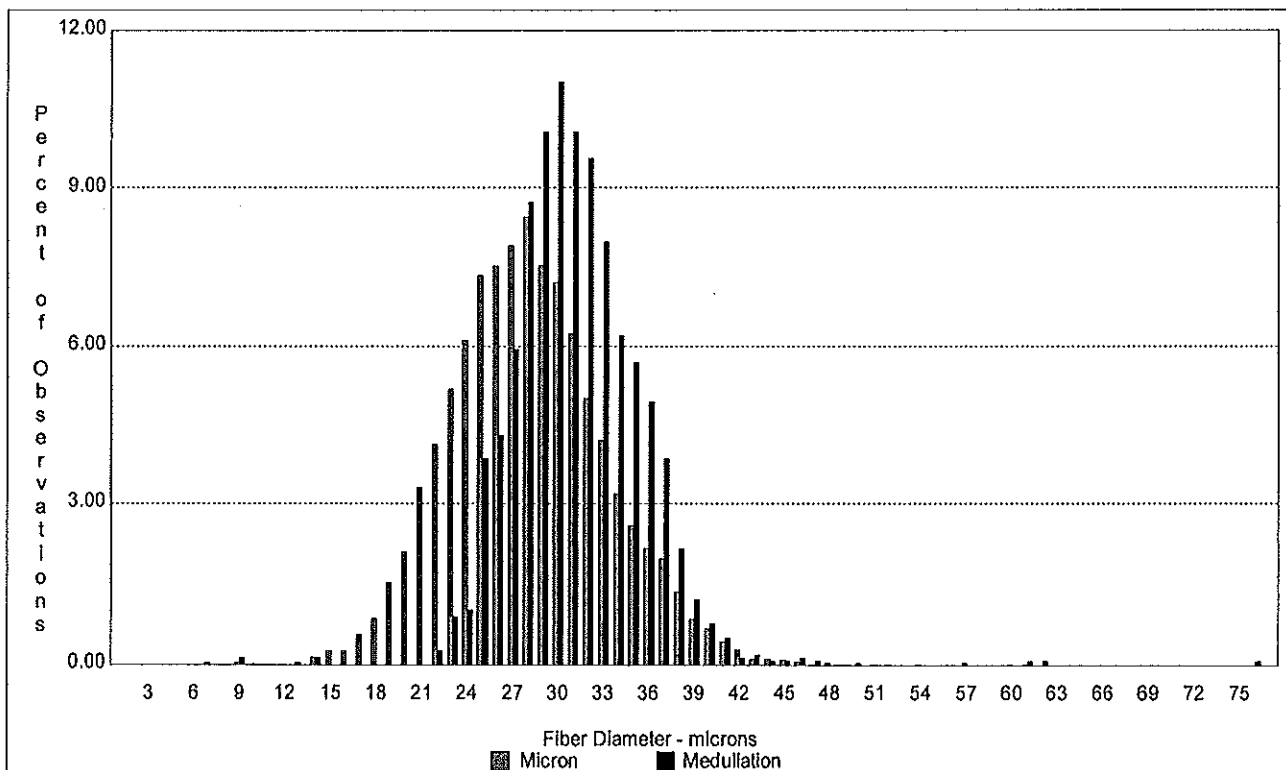

This Test Performed According to I.W.T.O Method 47